


DIAMOND[®]

DIAGNOSTICS

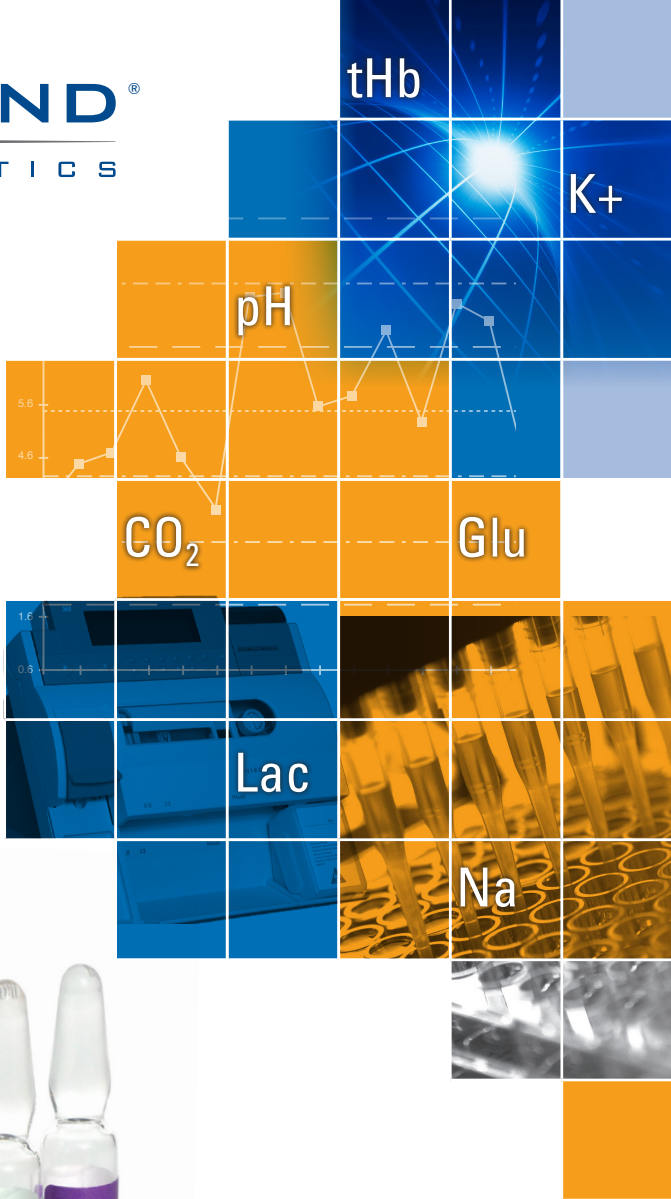

MISSION[®]

Quality Controls for Blood Gas, ISE, Coox and Metabolite systems



Mission CONTROL™

Aqueous Based Controls

- Assayed for pH, pCO₂, pO₂, Na⁺, K⁺, Ca⁺⁺, Cl⁻, Li⁺, tCO₂
- 36 month stability room temperature
- 60 second Open Vial Stability

Mission TRINITY™

Aqueous Based Control with Dyes and Metabolites

- Assayed for pH, pCO₂, pO₂, Na⁺, K⁺, Ca⁺⁺, Cl⁻, Li⁺, Glucose, Lactate, tHb, sO₂, MetHb, COHb, Hb, O₂Hb
- 36 month stability when refrigerated
- 60 second Open Vial Stability

Mission COMPLETE™

Aqueous Based CVM Linearity Control

- Assayed for pH, pCO₂, pO₂, Na⁺, K⁺, Ca⁺⁺, Cl⁻, Li⁺, Glucose, Lactate
- 36 month stability when refrigerated
- 60 second Open Vial Stability
- 5 Levels with Color Code Ampules covering analyzer significant ranges

Mission WebSTAT™

- Secure, Easy to Use Web-Based Statistics program offered
- Month to Date, Year to Date and Peer Group Reference
- Levy-Jennings Plots provided monthly
- Linear Regression Graphs supplied on-line for Complete Customers

Assayed Instrumentation


Abbott I-Stat
Idexx
Instrumentation Laboratory
ITC (formerly Diametrics)
Medica
Nova Biomedical
OPTI Medical
Radiometer
Roche Diagnostics (formerly AVL)
Siemens Diagnostics (formerly Bayer)

Assayed Instrumentation

Instrumentation Laboratory
Radiometer
Roche Diagnostics (formerly AVL)
Siemens Diagnostics (formerly Bayer)

Assayed Instrumentation

Abbott I-Stat
Instrumentation Laboratory
ITC (formerly Diametrics)
Nova Biomedical
OPTI Medical
Radiometer
Roche Diagnostics (formerly AVL)
Siemens Diagnostics (formerly Bayer)

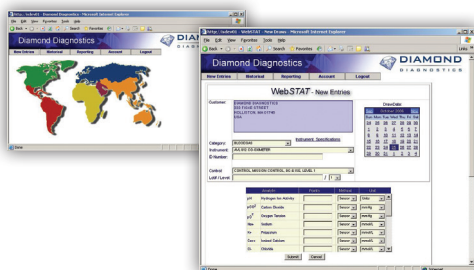

The names of manufacturers, their instruments, and their products referred to herein may be protected by trademark or other law and are used herein solely for purpose of reference. Diamond Diagnostics expressly disclaims any affiliation with them or sponsorship by them. For current regulatory status on products within this catalog, please contact your sales representative.